

Diode Laser Hygrometer Measurements of H₂O(v) During INTEX-A

Glenn S. Diskin and Glen W. Sachse
NASA Langley Research Center

James R. Podolske
NASA Ames Research Center

Thomas A. Slate and Mauro Rana
Swales Aerospace





INTEX-A Data Meeting
Virginia Beach, VA
March 29, 2005




Outline

- DLH Instrument
 - Operation
 - Status during INTEX-A
 - Calibration
- DLH Intercomparisons
 - P3 Intercomparisons
 - DC-8 Project Water
- Data Status

DLH Instrument Overview

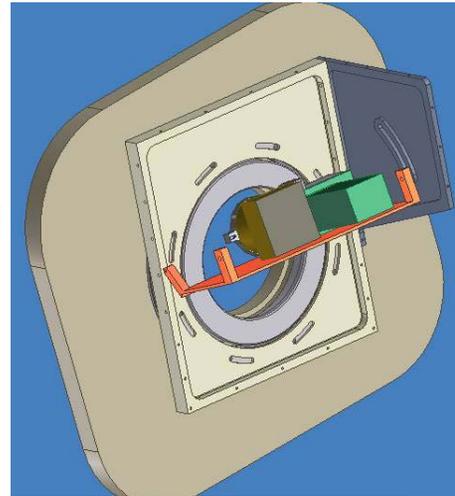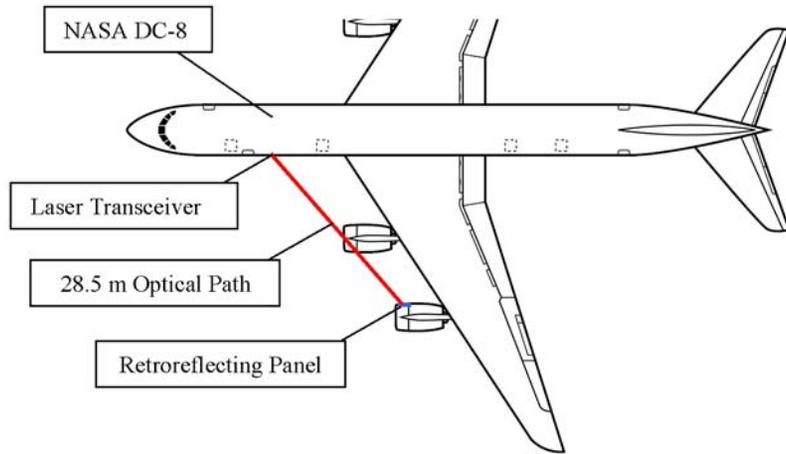


Schematic from Inside DC-8

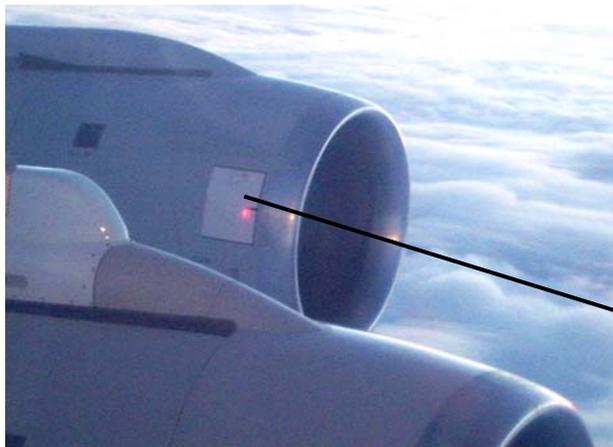

DLH Transceiver From Outside DC-8

Retroreflector Panel on Engine

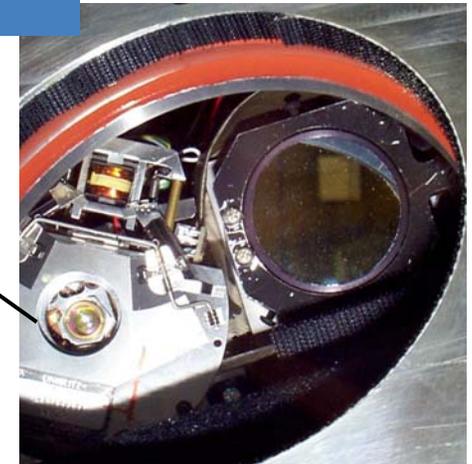

DLH: the NASA Langley / Ames Diode Laser Hygrometer

- Tunable diode laser hygrometer operating in the 1.4 μm spectral region
- Wavelength modulation at ~ 3 kHz
 - data analysis based on 2F demodulation, normalized by signal power
- Line-locked to absorption line in low-pressure reference cell
- Uses one of three absorption lines, depending on conditions (primarily altitude)
- Double-pass external path configuration
 - “mirror” is panel of retroreflecting road sign material, mounted on the outboard engine
 - sample volume is primarily outside of aircraft boundary layer
 - Internal optical path is purged with dry air
 - no inlet effects, such as condensation, evaporation, etc.
 - long path-length (28.5 m on DC-8), combined with line-locked, second harmonic detection allow good sensitivity and rapid time response
 - normalization by return power allows measurements to be made within clouds

New and Improved for INTEX-A !

- DLH operation, in-flight calibrations, and data acquisition controlled by 2U Windows/LabVIEW system
- Analog Lock-In Amplifier replaced by computer-based digital Lock-In
 - Full absorption lineshape available for post-mission analysis
- Data rate: 100 independent samples/sec
 - 1 second data submitted to archive; higher rate available on request
 - system bandwidth limited to ~20/sec by volume of sampled external path
- Better solar background rejection using frequent offset measurement
- Preliminary values of water vapor concentration reported in-flight

Instrument Status during INTEX-A

- DLH operational on every flight
- Data provided:
 - 95.5% of 1 second periods
 - 96.6% of 10 second periods
 - 97.5% of 1 minute periods
- Currently analyzing return signal power variations during mission
 - Measurement of attenuation by clouds at 1.4 μm
 - Hope to extend this to visible wavelengths and fly prototype during INTEX-B

Instrument Status, continued

- DLH data header contains an error

INSTRUMENT_INFO: Diode Laser Hygrometer - external path in-situ water vapor

DATA_INFO: Water Vapor **Dry** Mixing Ratio in ppmv

UNCERTAINTY: H₂O(v) = 5%

- Header should read:

INSTRUMENT_INFO: Diode Laser Hygrometer - external path in-situ water vapor


DATA_INFO: Water Vapor **Wet** Mixing Ratio in ppmv

UNCERTAINTY: H₂O(v) = 5%

We report $p_{\text{H}_2\text{O}}/p_{\text{air}} \times 10^6$, rather than $p_{\text{H}_2\text{O}}/(p_{\text{air}} - p_{\text{H}_2\text{O}}) \times 10^6$

- Update will be made to archived data this week




Laboratory Calibration of DLH

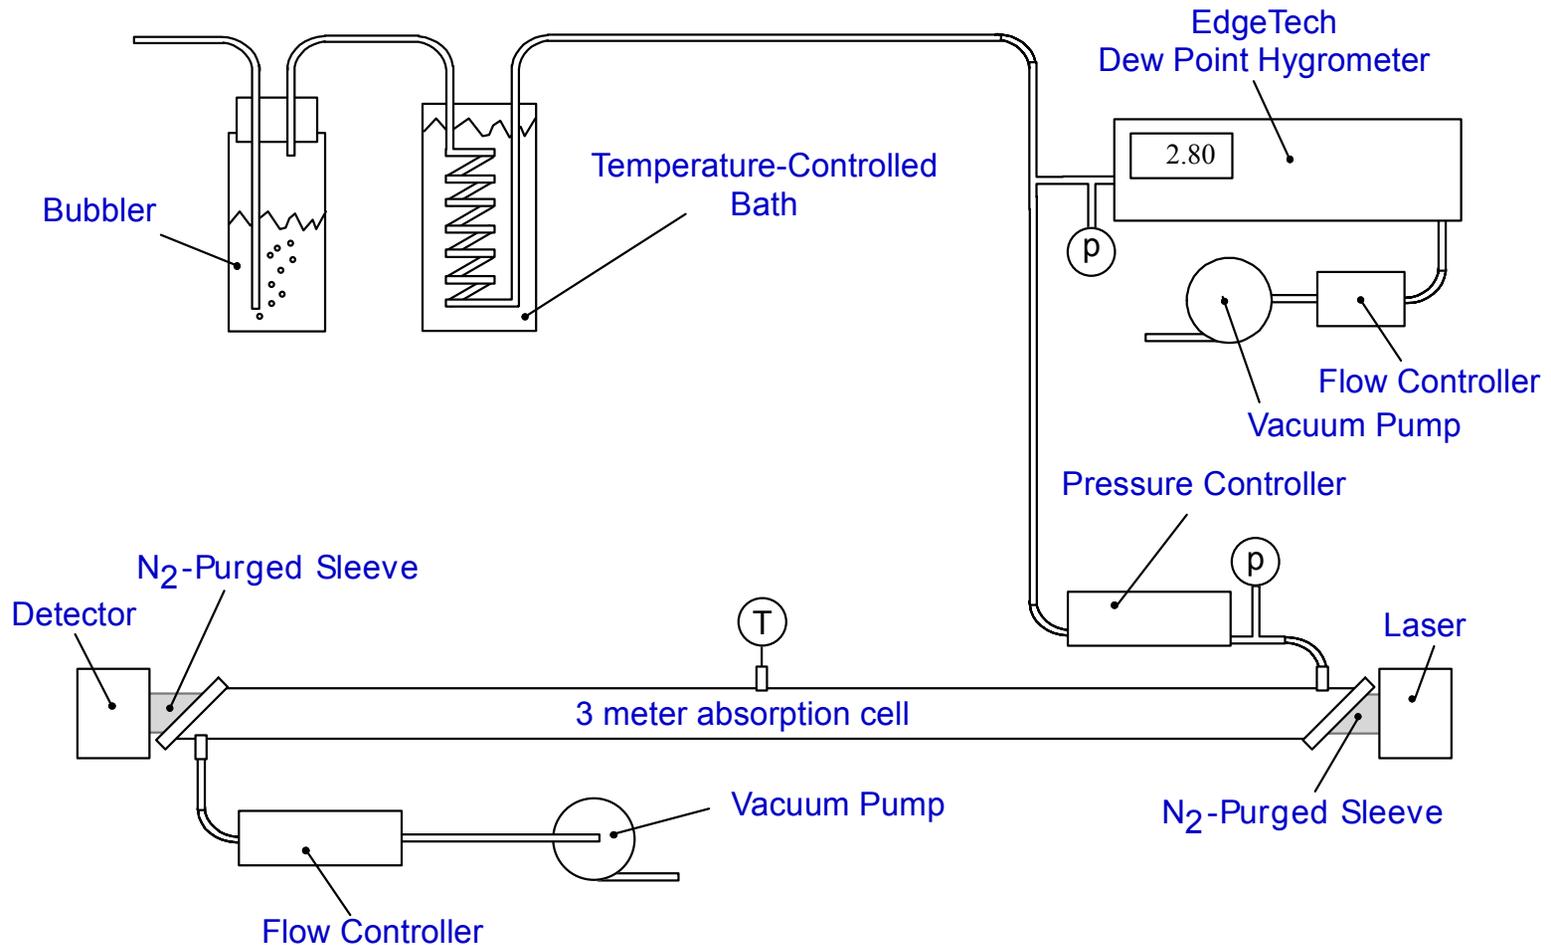

DLH Calibration Methodology

- External path prevents calibration of installed instrument, except at 'nature's choice' conditions
- Lab calibrations conducted at several values of pressure and water vapor concentration, to quantify laser characteristics and absorption line parameters
 - NIST-traceable chilled mirror hygrometer samples calibration mixture
- Spectral model developed which predicts harmonic lineshape
- Project-supplied static temperature and pressure are used convert measured signal into mixing ratio

H₂O Comparison

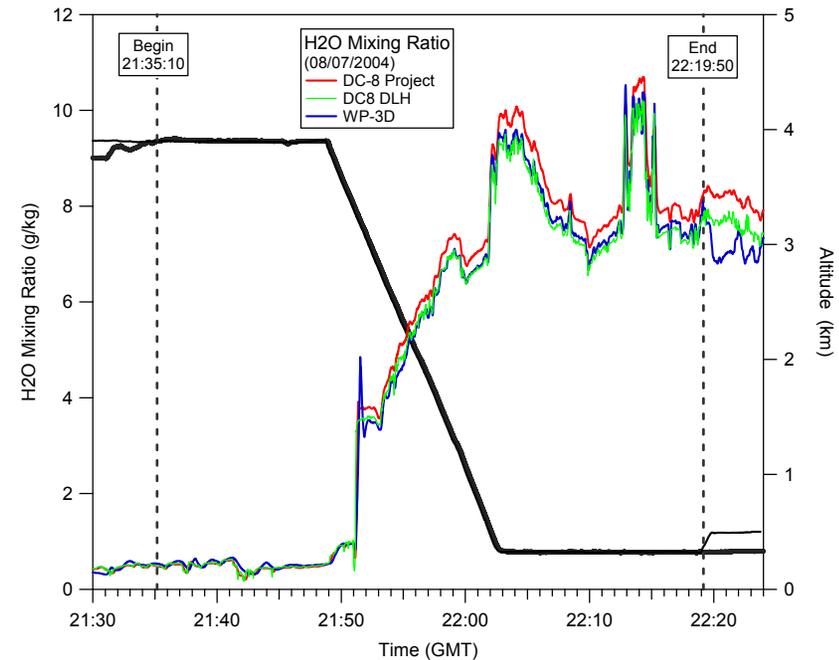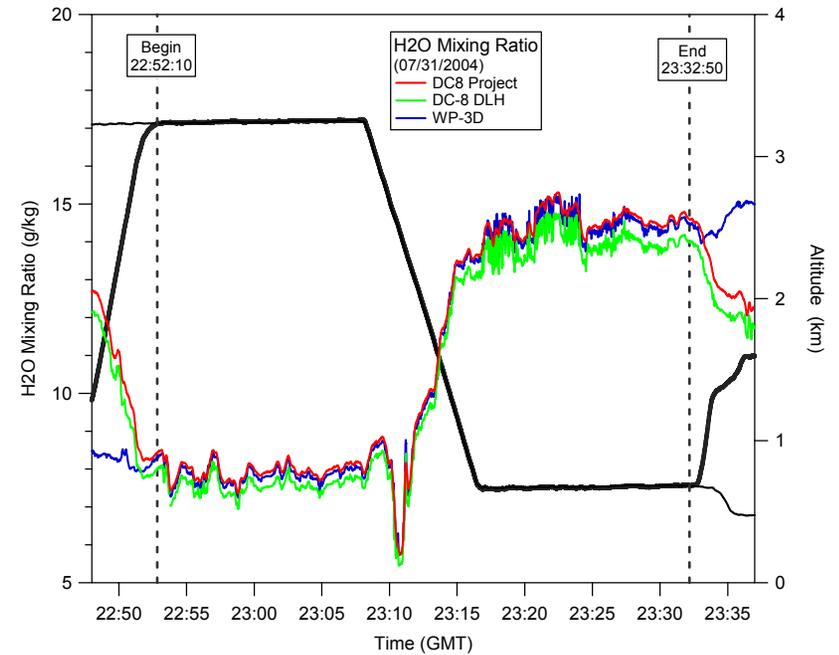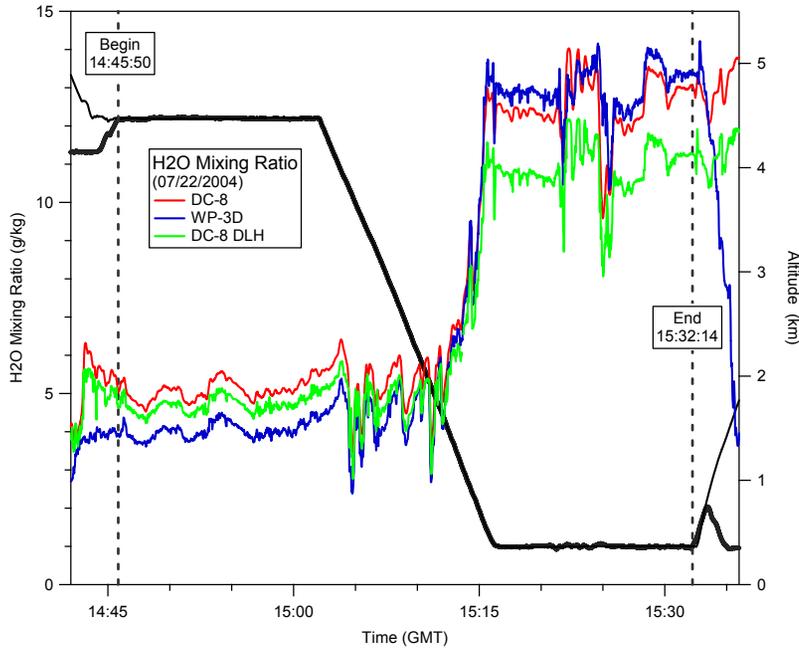

R^2 values: 0.99


DC-8 DLH vs. WP-3D Slope:

0.70 – 0.97


DC-8 Project vs. WP-3D Slope:

0.84 – 1.05

DLH vs. Project Water Vapor during INTEX-A

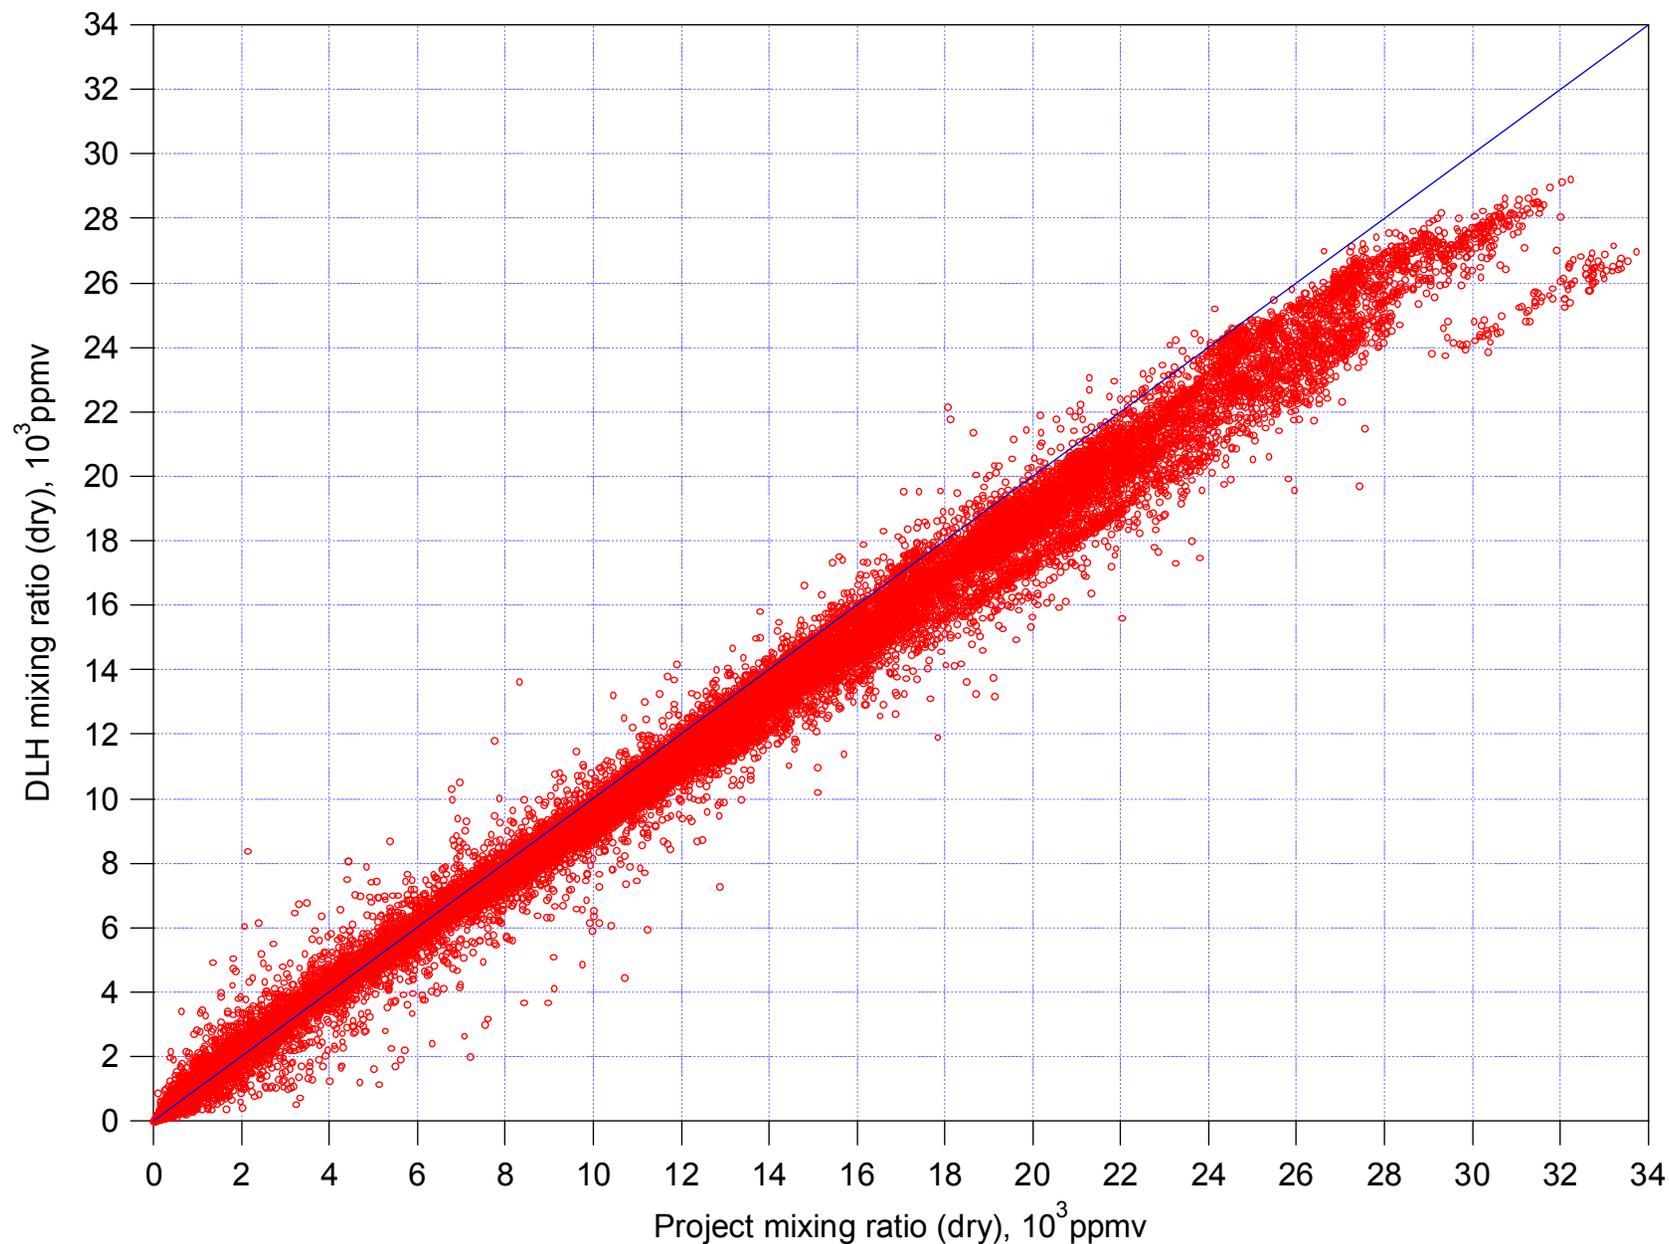


Altitude-Specific Histograms of DLH/Project Water Vapor Ratio

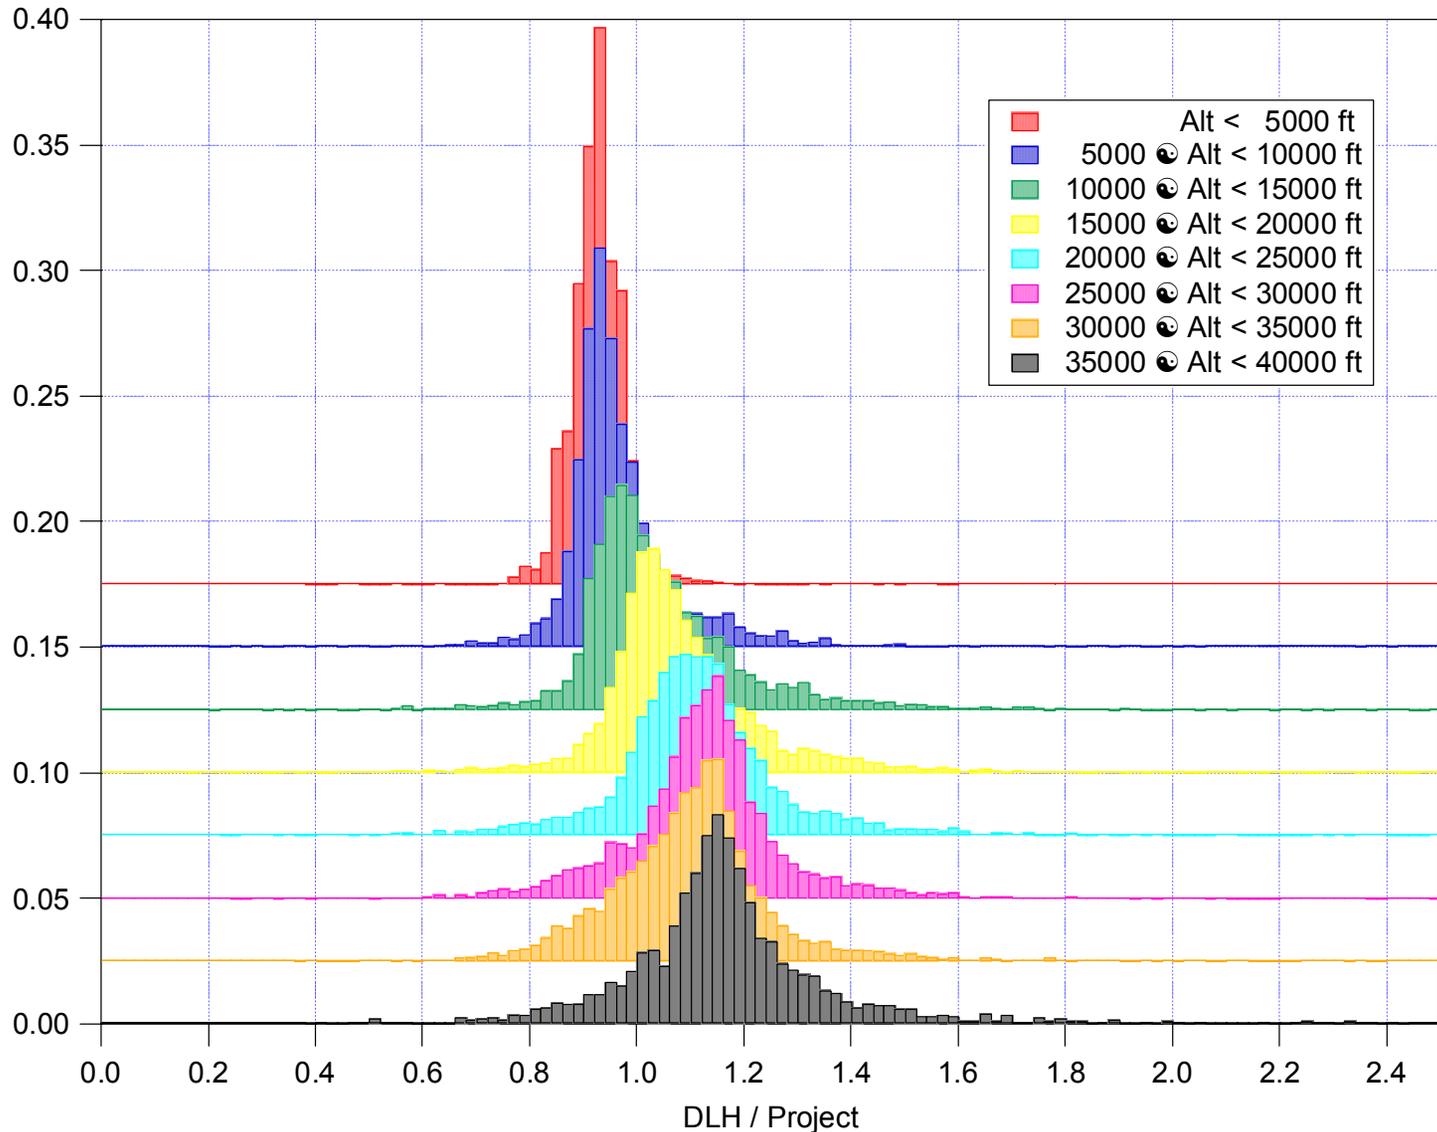

DLH vs. Project Water Vapor Comparison

Low Altitude, DLH using Weak Absorption Line

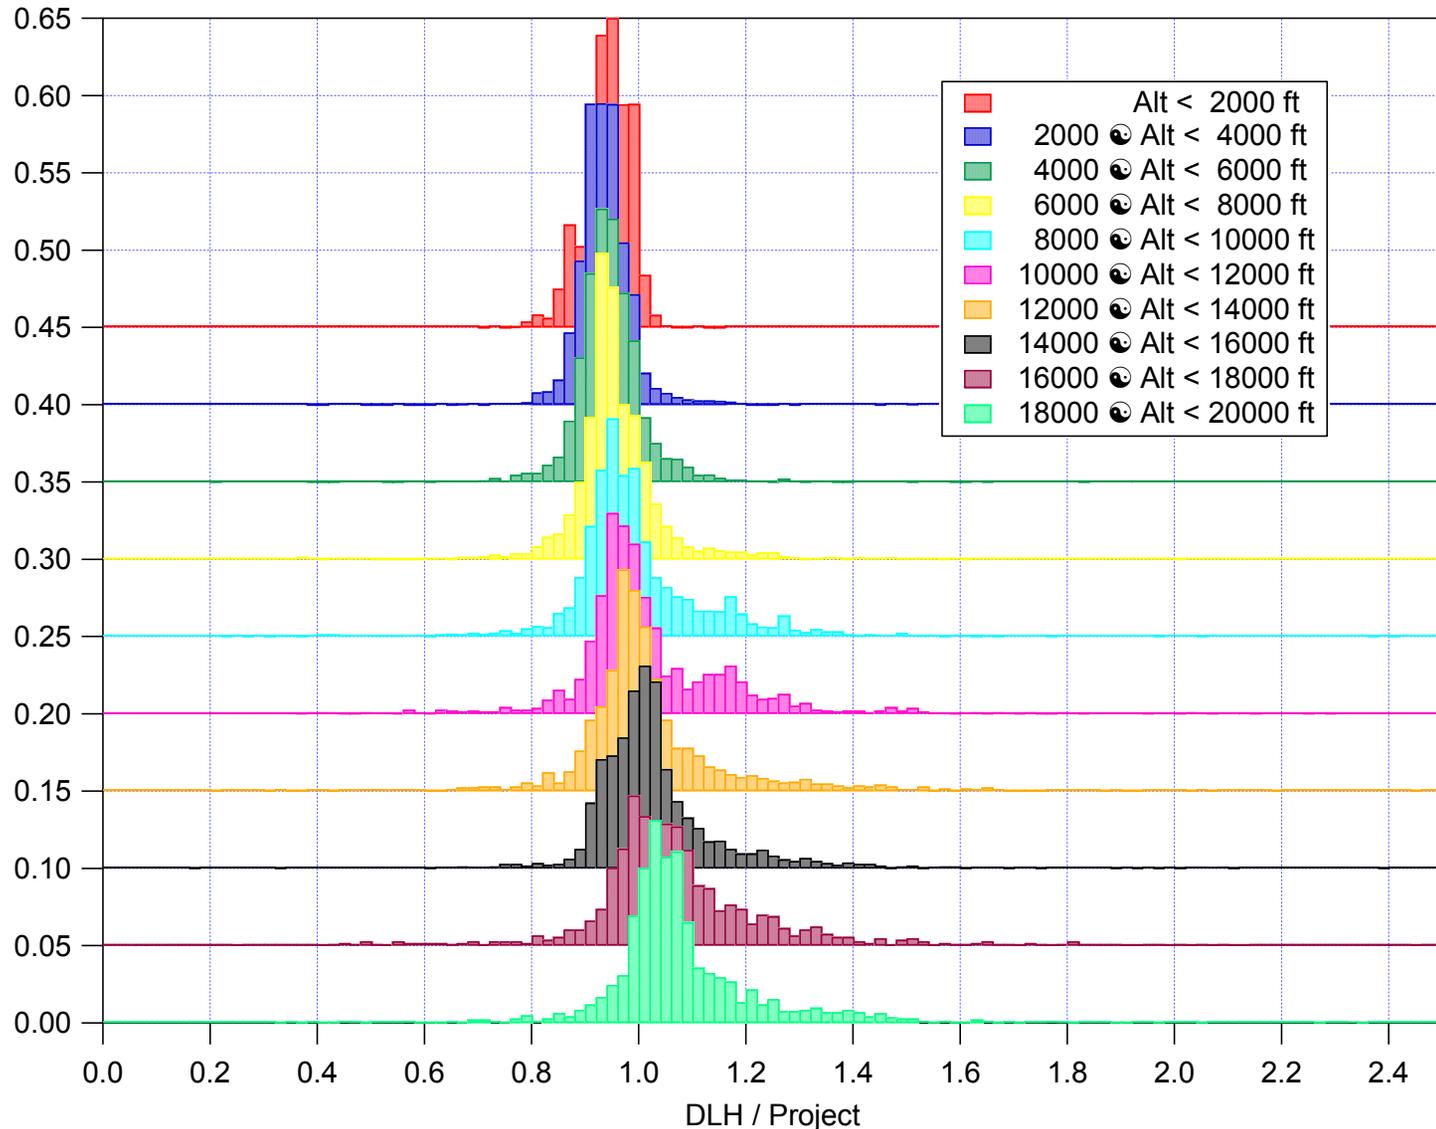

Examination of DLH Data

- DLH vs Project Water Vapor shows consistent trend at low altitudes / high water vapor concentrations
- DLH tends to be ~6% lower than project water at low altitudes, the difference decreasing as altitude increases
- For altitude < 20 kft, most DLH data taken using (new) weak absorption line
- Examination of flight data does not show any line-specific bias
- Examination of calibration data has not yet yielded any inconsistency within the weak line sets, or between the weak line and stronger line sets
- We will continue to examine our calibration and data analysis methodologies

Summary

- DLH performed successfully during entire INTEX-A mission
- DLH mixing ratio compared very well with P-3 and DC-8 project water during two of the three intercomparisons, less well during the July 22 intercomparison
- DLH and DC-8 project water mixing ratios differ by ~6% at the lowest altitudes; cause as yet undetermined
- DLH data file header contains definition error; will be fixed soon!